

LSBio™ Human F8 / FVIII / Factor VIII ELISA Kit

Catalog No. LS-F10415

User Manual

**Please Read the Manual Carefully
Before Starting your Experiment**



For research use only. Not approved for use in humans or for clinical diagnosis.

Human Coagulation Factor VIII Total Antigen ELISA Kit

Catalog # LS-F10415 Strip well
format. Reagents for up to 96 tests.

Rev: December 2014

INTENDED USE

This human coagulation Factor VIII antigen assay is intended for the quantitative determination of total Factor VIII antigen in human plasma. **For research use only.**

BACKGROUND

Factor VIII (aka Factor VIII:C or Antihemophilic Globulin) is a glycoprotein zymogen that circulates in a stabilized non-covalent complex with von Willebrand Factor (vWF) [1]. Following activation by thrombin or Factor Xa, Factor VIIIa dissociates from vWF and catalyzes the activation of Factor X by Factor IXa in the amplification phase of coagulation [2]. Factor VIIIa activity is quickly decreased by spontaneous dissociation and proteolytic degradation by activated Protein C, Factor Xa and Factor IXa [3]. Hemophilia A is caused by mutations in the Factor VIII gene; a majority of patients have decreased Factor VIII plasma levels while 5% of patients have normal levels of nonfunctioning protein [4].

ASSAY PRINCIPLE

Human Factor VIII will bind to the affinity purified capture antibody coated on the microtiter plate. After appropriate washing steps, biotin labeled anti-human

Factor VIII primary antibody binds to the captured protein. Excess primary antibody is washed away and bound antibody is reacted with peroxidase conjugated streptavidin. Following an additional washing step, TMB substrate is used for color development at 450nm. A standard calibration curve is prepared along with the samples to be measured using dilutions of human plasma. Color development is proportional to the concentration of Factor VIII in the samples.

STANDARD CALIBRATION

The Factor VIII level in the human plasma standard provided is calibrated against a secondary standard that is referenced to the WHO or ISTH International Standard.

REAGENTS PROVIDED

- **96-well antibody coated microtiter strip plate** (removable wells 8x12) containing anti-human factor VIII antibody, blocked and dried.
- **10X Wash buffer:** 1 bottle of 50ml
- **Human Factor VIII standard:** 1 vial lyophilized plasma
- **Anti-human Factor VIII primary antibody:** 1 vial lyophilized polyclonal antibody
- **Horseradish peroxidase-conjugated streptavidin:** 1 vial concentrated HRP labeled streptavidin
- **TMB substrate solution:** 1 bottle of 10ml solution

STORAGE AND STABILITY

Store all kit components at 4°C upon arrival. Return any unused microplate strips to the plate pouch with desiccant. Reconstituted standards and primary may be stored at -80°C for later use. Do not freeze-thaw the standard and primary antibody more than once. Store all other unused kit components at 4°C. This kit should not be used beyond the expiration date.

OTHER REAGENTS AND SUPPLIES REQUIRED

- Microtiter plate shaker capable of 300 rpm uniform horizontally circular movement
- Manifold dispenser/aspirator or automated microplate washer
- Microplate reader capable of measuring absorbance at 450 nm
- Pipettes and Pipette tips
- Deionized or distilled water
- Polypropylene tubes for dilution of standard
- Paper towels or laboratory wipes
- 1N H₂SO₄ or 1N HCl
- Bovine Serum Albumin Fraction V (BSA)
- Tris(hydroxymethyl)aminomethane (Tris)
- Sodium Chloride (NaCl)

PRECAUTIONS

- FOR LABORATORY RESEARCH USE ONLY. NOT FOR DIAGNOSTIC USE.
- Do not mix any reagents or components of this kit with any reagents or components of any other kit. This kit is designed to work properly as provided.
- Always pour peroxidase substrate out of the bottle into a clean test tube. Do not pipette out of the bottle as contamination could result.
- Keep plate covered except when adding reagents, washing, or reading.
- DO NOT pipette reagents by mouth and avoid contact of reagents and specimens with skin.
- DO NOT smoke, drink, or eat in areas where specimens or reagents are being handled.

PREPARATION OF REAGENTS

- TBS buffer:** 0.1M Tris, 0.15M NaCl, pH 7.4
- Blocking buffer (BB):** 3% BSA (w/v) in TBS
- 1X Wash buffer:** Dilute 50ml of 10X wash buffer concentrate with 450ml of deionized water

SAMPLE COLLECTION

Collect plasma using EDTA or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. Assay immediately or aliquot and store at $\leq -20^{\circ}\text{C}$. Avoid repeated freeze-thaw cycles.

ASSAY PROCEDURE

Perform assay at room temperature. Vigorously shake plate (300rpm) at each step of the assay.

Preparation of Standard

Reconstitute standard by adding 1ml of deionized water directly to the vial and agitate gently to completely dissolve contents. This will result in a 0.92 IU/ml plasma standard.

Dilution table for preparation of human Factor VIII standard:

Factor VIII concentration (IU/ml)	Dilutions
0.92	From vial
0.46	500 μl (BB) + 500 μl (0.92 IU/ml)
0.23	500 μl (BB) + 500 μl (0.43 IU/ml)
0.115	500 μl (BB) + 500 μl (0.23 IU/ml)
0.0575	500 μl (BB) + 500 μl (0.115 IU/ml)
0.0288	500 μl (BB) + 500 μl (0.0575 IU/ml)
0.0144	500 μl (BB) + 500 μl (0.0288 IU/ml)
0.0072	500 μl (BB) + 500 μl (0.0144 IU/ml)
0.0036	500 μl (BB) + 500 μl (0.0072 IU/ml)
0.0018	500 μl (BB) + 500 μl (0.0036 IU/ml)
0	500 μl (BB) Zero point to determine background

NOTE: DILUTIONS FOR THE STANDARD CURVE AND ZERO STANDARD MUST BE MADE AND APPLIED TO THE PLATE IMMEDIATELY.

Standard and Unknown Addition

Remove microtiter plate from bag and add 100 μl Factor VIII standards (in duplicate) and unknowns to wells. Carefully record position of standards and unknowns. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300 μl wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

NOTE: The assay measures Factor VIII antigen in the 0.0018-0.92 IU/ml range. 1:50 and 1:100 dilutions

for normal plasma, or 1:4 and 1:8 dilutions for Haemophilic plasma, are suggested for best results.

Primary Antibody Addition

Reconstitute primary antibody by adding 10ml of blocking buffer directly to the vial and agitate gently to completely dissolve contents. Add 100 μl to all wells. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300 μl wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

Streptavidin-HRP Addition

Briefly centrifuge vial before opening. Dilute 2.5µl of HRP conjugated streptavidin into 2.5ml blocking buffer to generate a 1:1,000 dilution. Add 0.2ml of the 1:1,000 dilution to 9.8ml of blocking buffer to generate a 1:50,000 dilution. Add 100µl of the 1:50,000 dilution to all wells. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300µl wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

Substrate Incubation

Add 100µl TMB substrate to all wells and shake plate for 2-10 minutes. Substrate will change from colorless to different strengths of blue. Quench reaction by adding 50µl of 1N H₂SO₄ or HCl stop solution to all wells when samples are visually in the same range as the standards. Add stop solution to wells in the same order as substrate upon which color will change from blue to yellow. Mix thoroughly by gently shaking the plate.


Measurement

Set the absorbance at 450nm in a microtiter plate spectrophotometer. Measure the absorbance in all wells at 450nm. Subtract zero point from all standards and unknowns to determine corrected absorbance (A₄₅₀).

Calculation of Results

Plot A₄₅₀ against the amount of Factor VIII in the standards. Fit a straight line through the linear points of the standard curve using a linear fit procedure if unknowns appear on the linear portion of the standard curve. Alternatively, create a standard curve by analyzing the data using a software program capable of generating a four parameter logistic (4PL) curve fit. The amount of Factor VIII in the unknowns can be determined from this curve. If samples have been diluted, the calculated concentration must be multiplied by the dilution factor.

A typical standard curve (EXAMPLE ONLY):

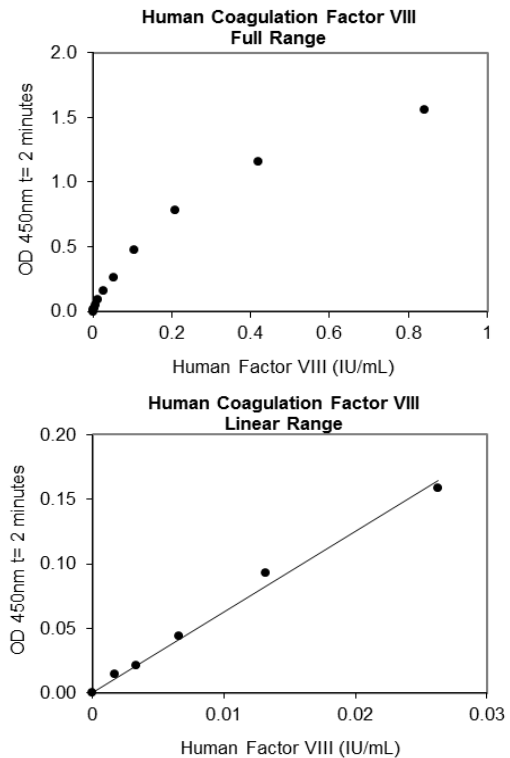

EXPECTED VALUES

The average normal plasma level of Factor VIII is defined as 1.0 IU/ml and the normal range is 0.4-1.8 IU/ml [5]. Hemaophilia A patients are classified by the following Factor VIII levels: 0.05-0.25 IU/ml = mild, 0.01-0.05 IU/ml = moderate, and <0.01 IU/ml = severe [6].

PERFORMANCE CHARACTERISTICS

Sensitivity: The minimum detectable dose (MDD) was determined by adding two standard deviations to the mean optical density value of eighteen zero standard replicates (range OD₄₅₀: 0.088-0.096) and calculating the corresponding concentration. The MDD was 0.00015 IU/ml.

Intra-assay Precision: These studies are currently in progress. Please contact us for more information.

Inter-assay Precision: These studies are currently in progress. Please contact us for more information.

Recovery: These studies are currently in progress. Please contact us for more information.

Linearity: These studies are currently in progress. Please contact us for more information.

Specificity: This antibody recognizes total human Factor VIII. Pooled normal plasma from mouse, rat, rabbit, pig, horse, guinea pig, dog, and sheep was assayed and no significant cross-reactivity was observed. Pooled normal plasma from cyno monkey, rhesus monkey and baboon was assayed and significant cross-reactivity was observed.

DISCLAIMER

This information is believed to be correct but does not claim to be all-inclusive and shall be used only as a guide. The supplier of this kit shall not be held liable for any damage resulting from handling of or contact with the above product.

Example of ELISA Plate Layout

96 Well Plate: 22 Standard wells, 74 Sample wells

	1	2	3	4	5	6	7	8	9	10	11	12
A	0	0.0015 IU/ml	0.003 IU/ml	0.006 IU/ml	0.012 IU/ml	0.024 IU/ml	0.048 IU/ml	0.096 IU/ml	0.19 IU/ml	0.39 IU/ml	0.77 IU/ml	
B	0	0.0015 IU/ml	0.003 IU/ml	0.006 IU/ml	0.012 IU/ml	0.024 IU/ml	0.048 IU/ml	0.096 IU/ml	0.19 IU/ml	0.39 IU/ml	0.77 IU/ml	
C												
D												
E												
F												
G												
H												

Important Note: During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. We recommend briefly centrifuging the vial to dislodge any liquid in the container's cap prior to opening.

Warning: This reagent may contain sodium azide and sulfuric acid. The chemical, physical, and toxicological properties of these materials have not been thoroughly investigated. Standard Laboratory Practices should be followed. Avoid skin and eye contact, inhalation, and ingestion. Sodium azide forms hydrazoic acid under acidic conditions and may react with lead or copper plumbing to form highly explosive metal azides. On disposal, flush with large volumes of water to prevent accumulation.

Returns, Refunds, Cancellations: Any problems with LifeSpan products must be reported to LifeSpan within 10 days of product receipt. The customer must obtain written authorization from LifeSpan before returning items. To request that goods be returned, please contact LifeSpan Technical Support. If an error by LifeSpan BioSciences results in shipment of an incorrect order, LifeSpan will, at its option, either ship a replacement order at no charge, or credit the customer's account for the original product shipped in error. Returns and cancellations may be subject to a 30% restocking fee.

Conditions & Warranty: All LifeSpan products are intended for Research Use Only and are not for use in human therapeutic or diagnostic applications. The information supplied with each product is believed to be accurate, but no warranty or guarantee is offered for the products, because the ultimate conditions of use are beyond LifeSpan's control. The information supplied with each product is not to be construed as a recommendation to use this product in violation of any patent, and LifeSpan will not be held responsible for any infringement or other violation that may occur with the use of its products. Under no event will LifeSpan be responsible for any loss of profit or indirect consequential damage, including, but not limited to, personal injuries resulting from use of these products. LifeSpan's liability to any user of Products for damages that do not result from any fault of the user, will be limited to replacement of the Product(s) only, and in no event shall LifeSpan's liability exceed the actual price received by LifeSpan for the Product(s) at issue. LifeSpan shall not be liable for any indirect, special, incidental or consequential damages. LIFESPAN FURTHER DISCLAIMS ANY AND ALL EXPRESS AND IMPLIED OR STATUTORY WARRANTIES WITH RESPECT TO THE PRODUCTS, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE. LifeSpan disclaims any and all responsibility for any injury or damage which may be caused by the fault of the user.

For research use only. Not approved for use in humans or for clinical diagnosis.



2401 Fourth Avenue Suite 900 Seattle, WA 98121

Tel: 206.374.1102

Fax: 206.577.4565

Technical.Support@LSBio.com